

Fig. 1

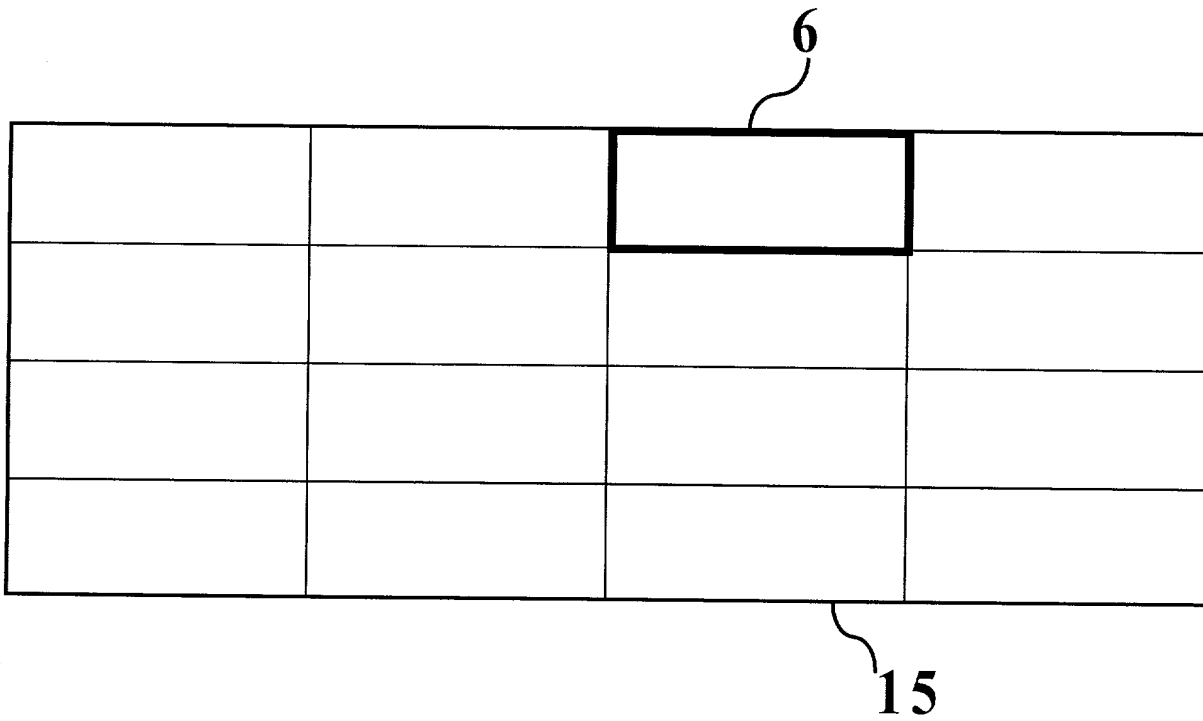


Fig. 2

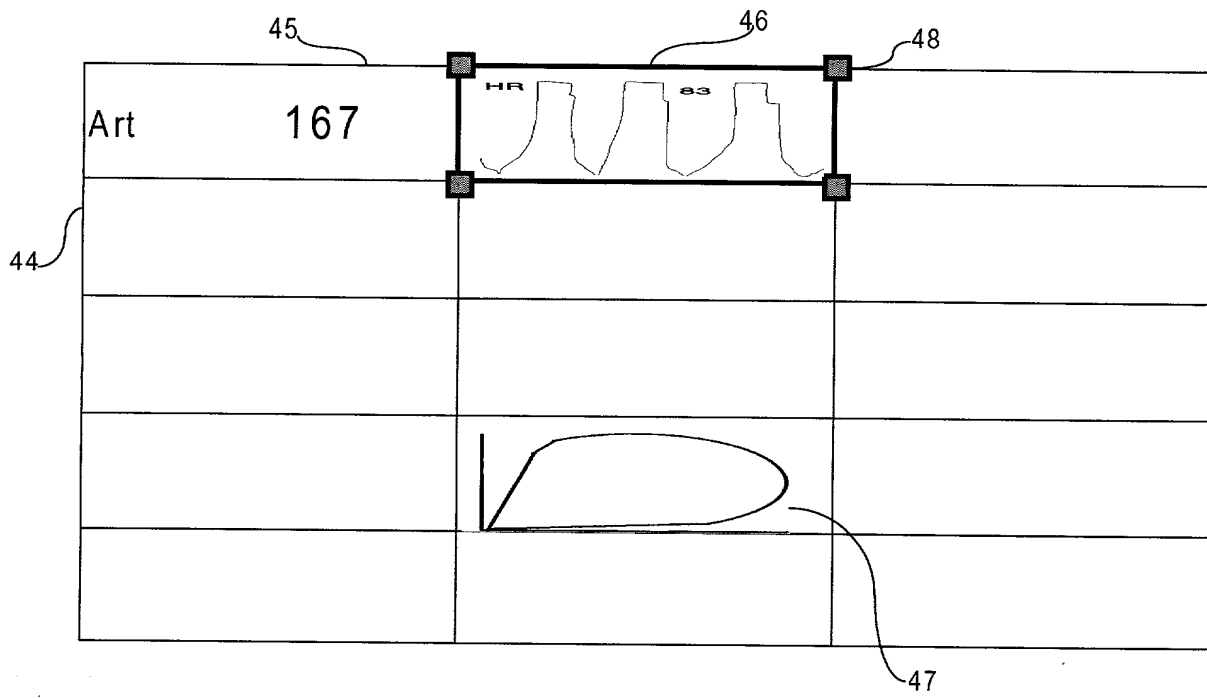



Fig. 3

[illegible]

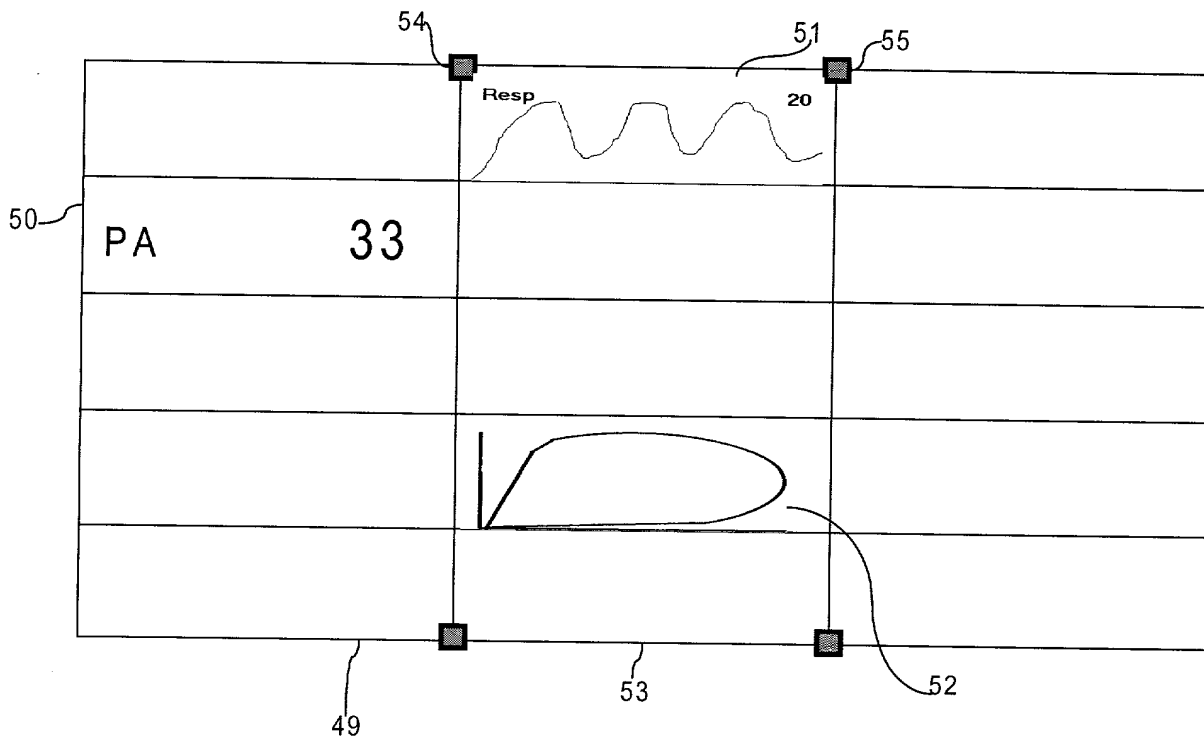


Fig. 5

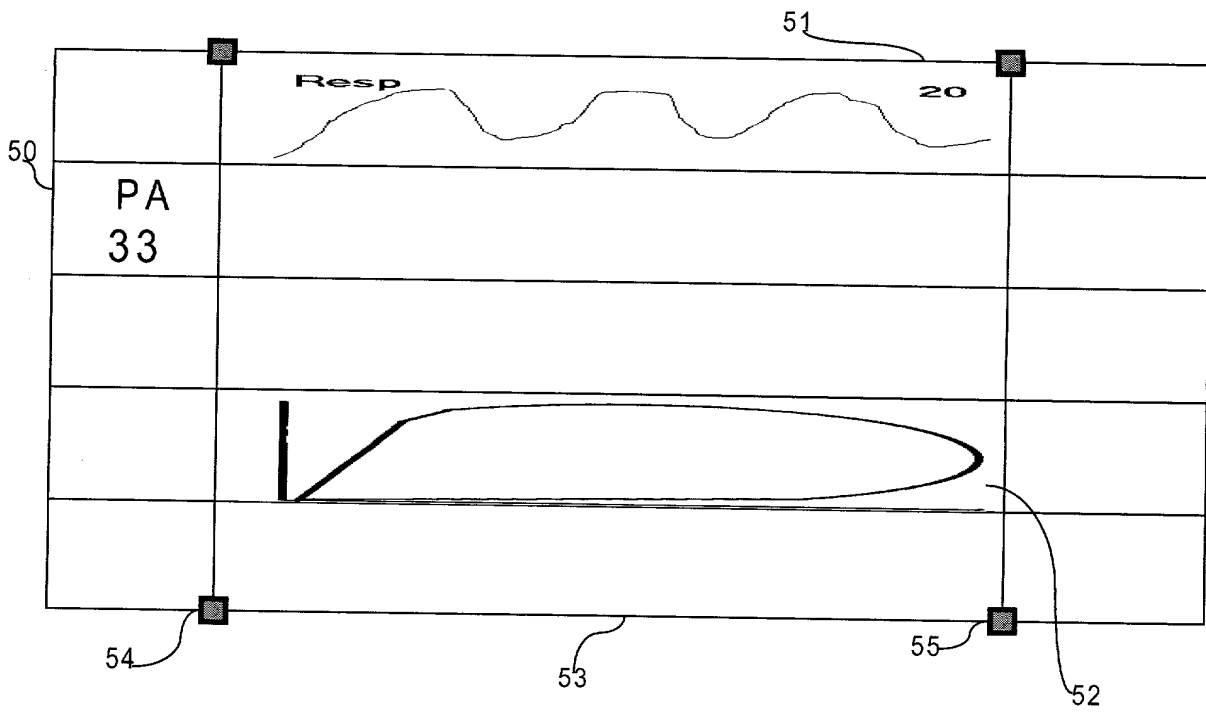


Fig. 6

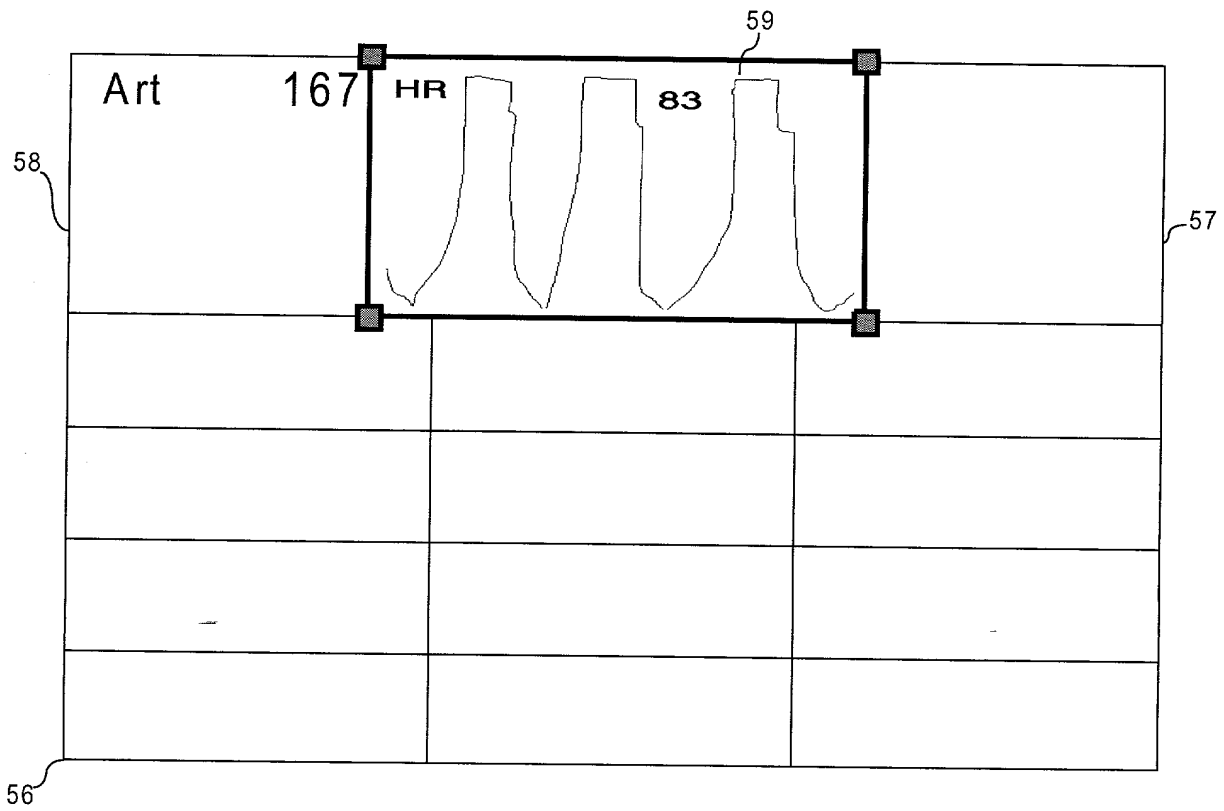


Fig. 7

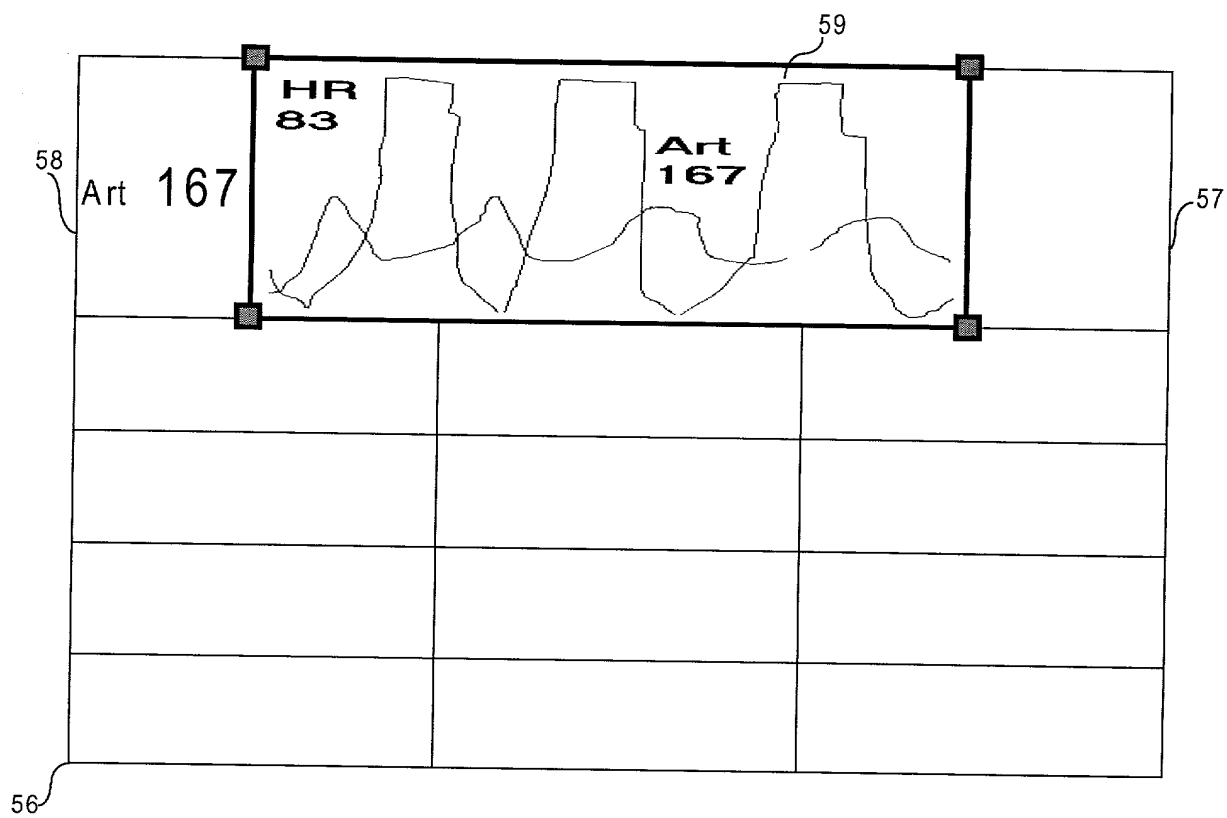


Fig. 8

FIG. 9 is a schematic diagram of a user interface for a medical device.

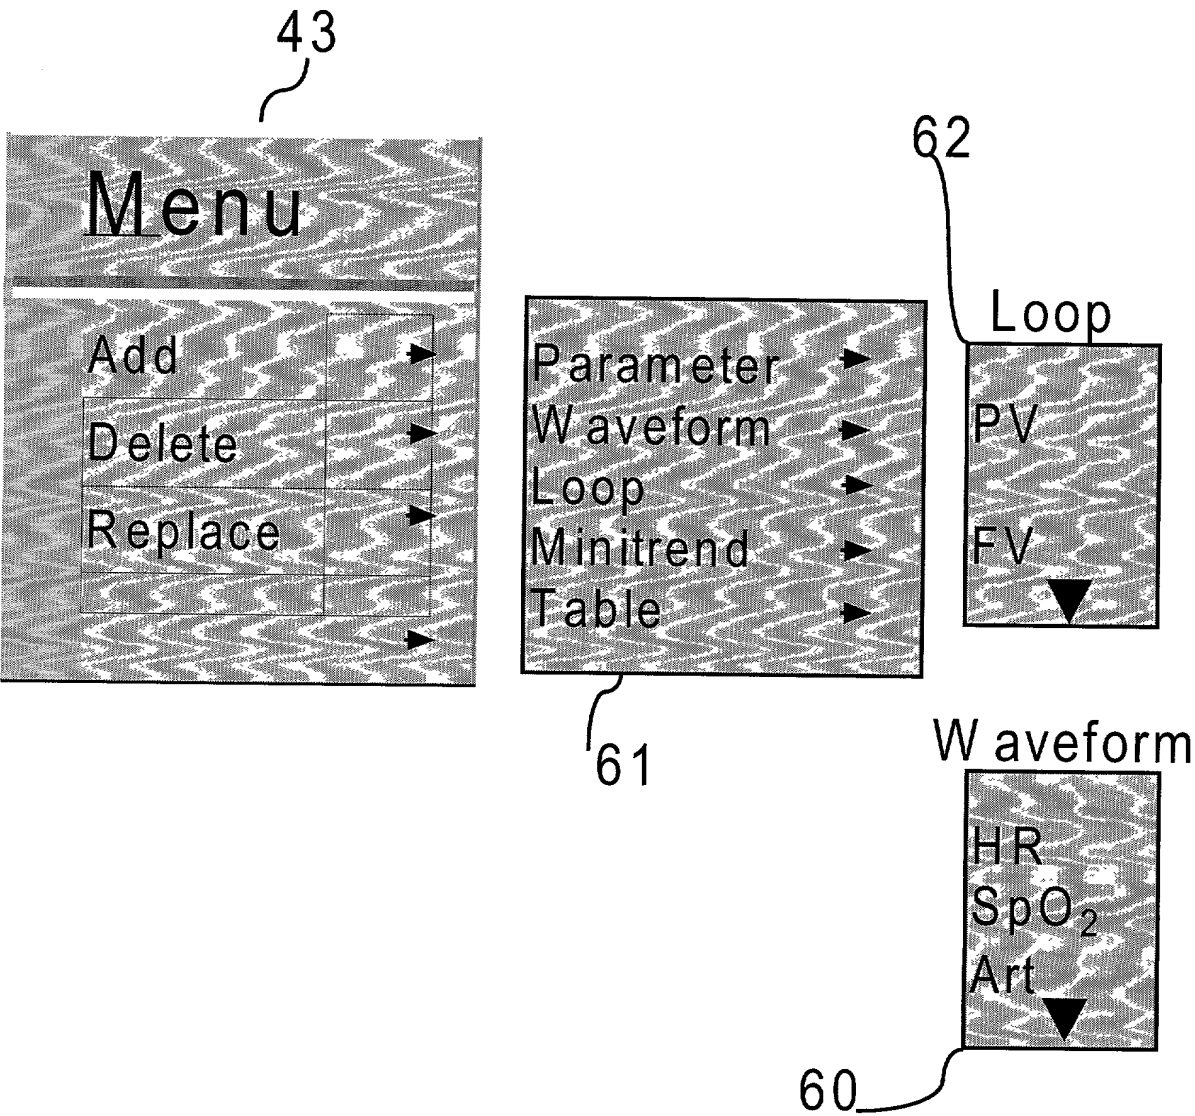


Fig. 9

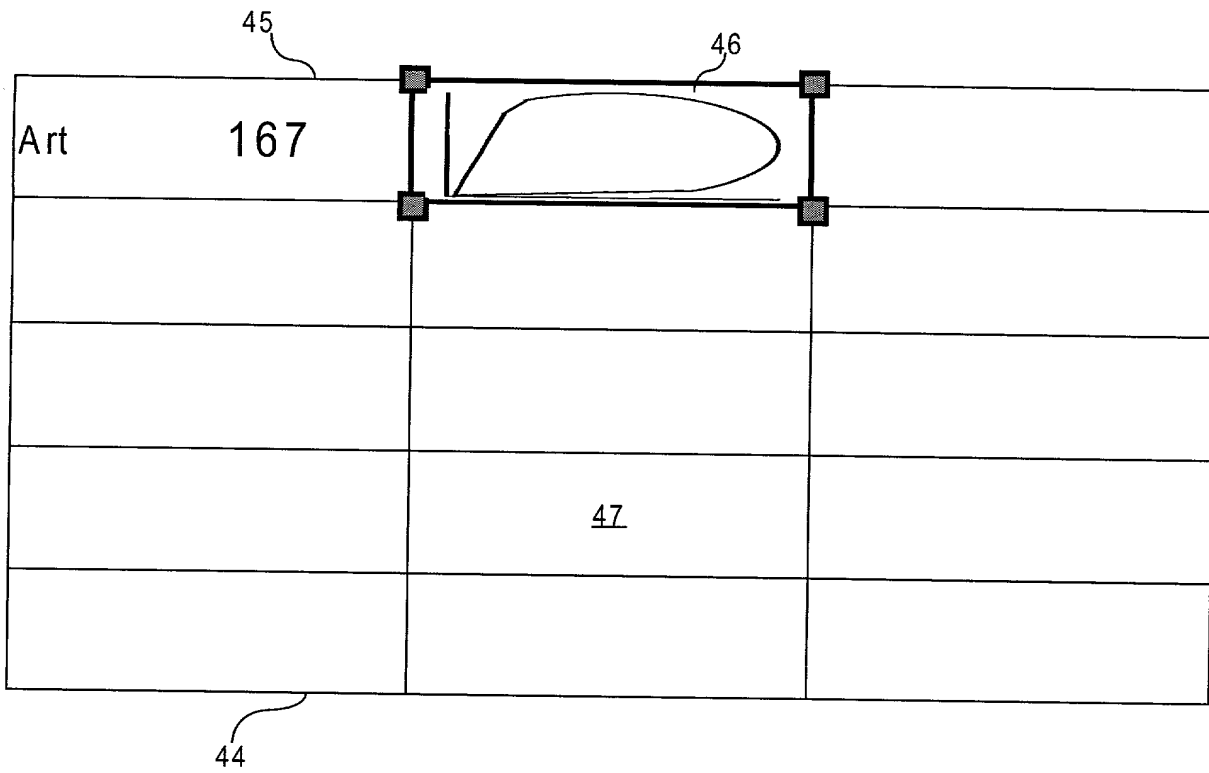


Fig. 10

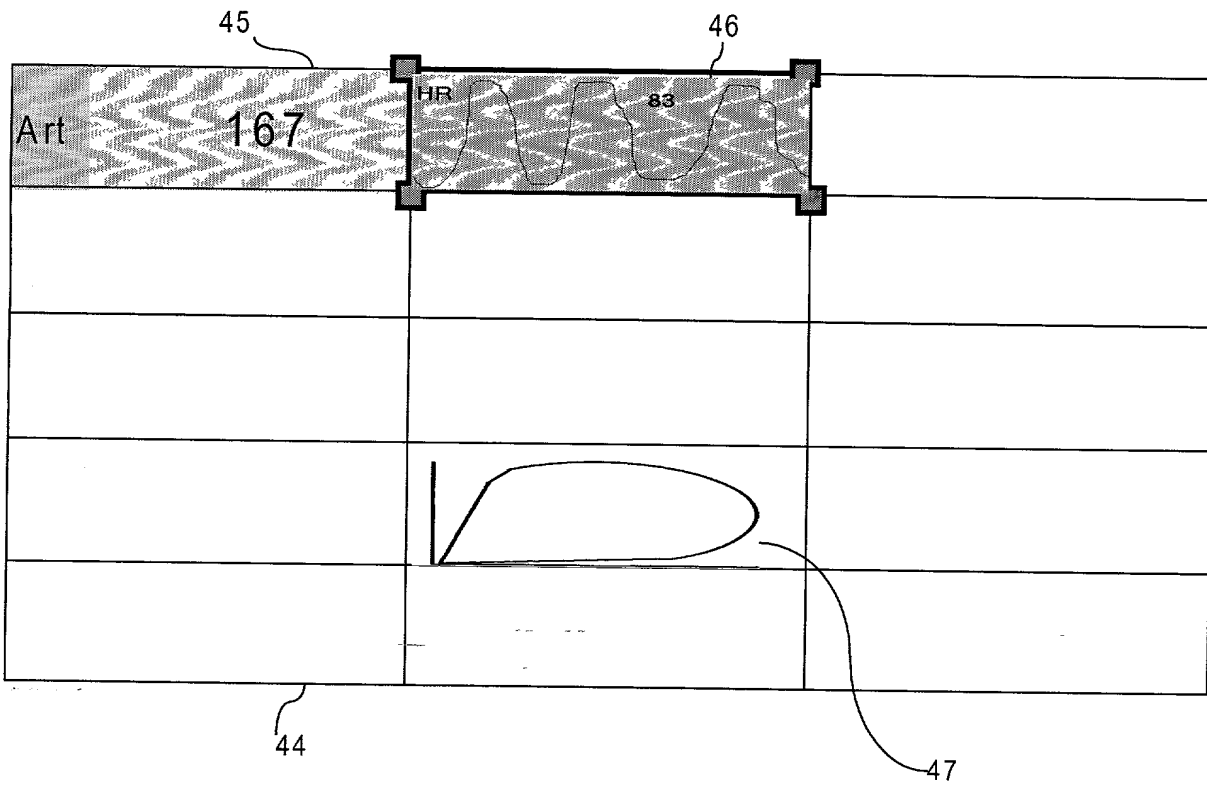


Fig. 11


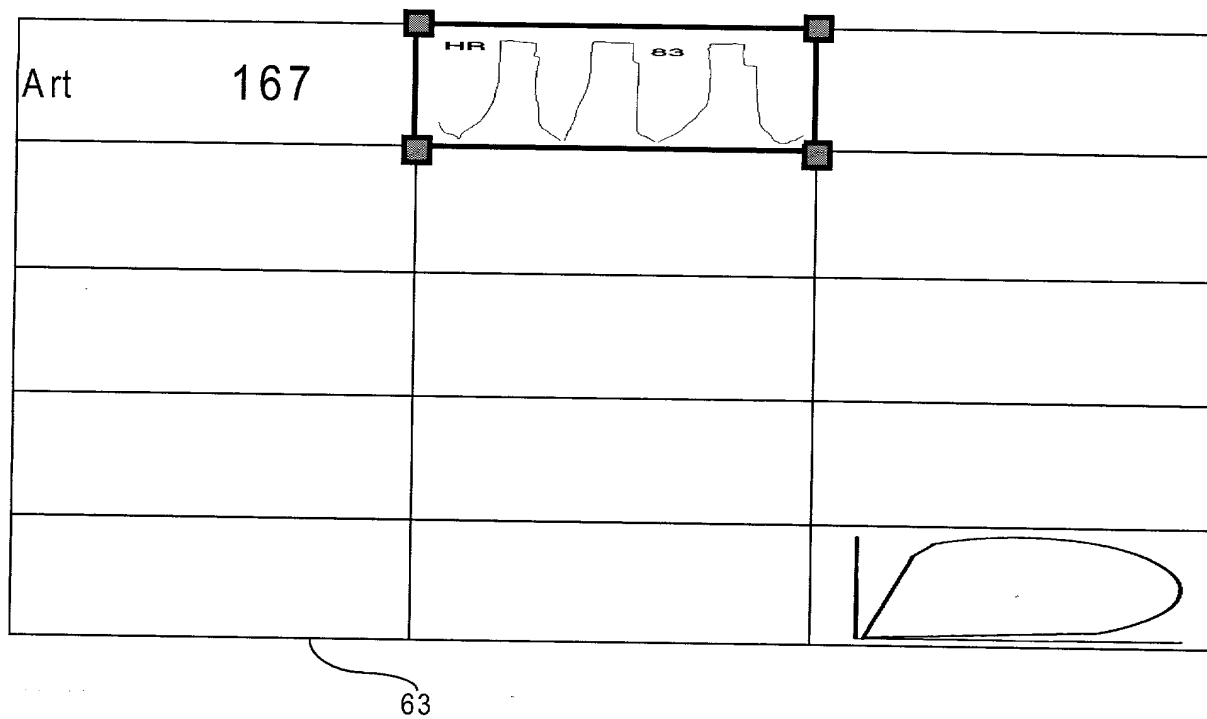


Fig. 12

FIG. 12

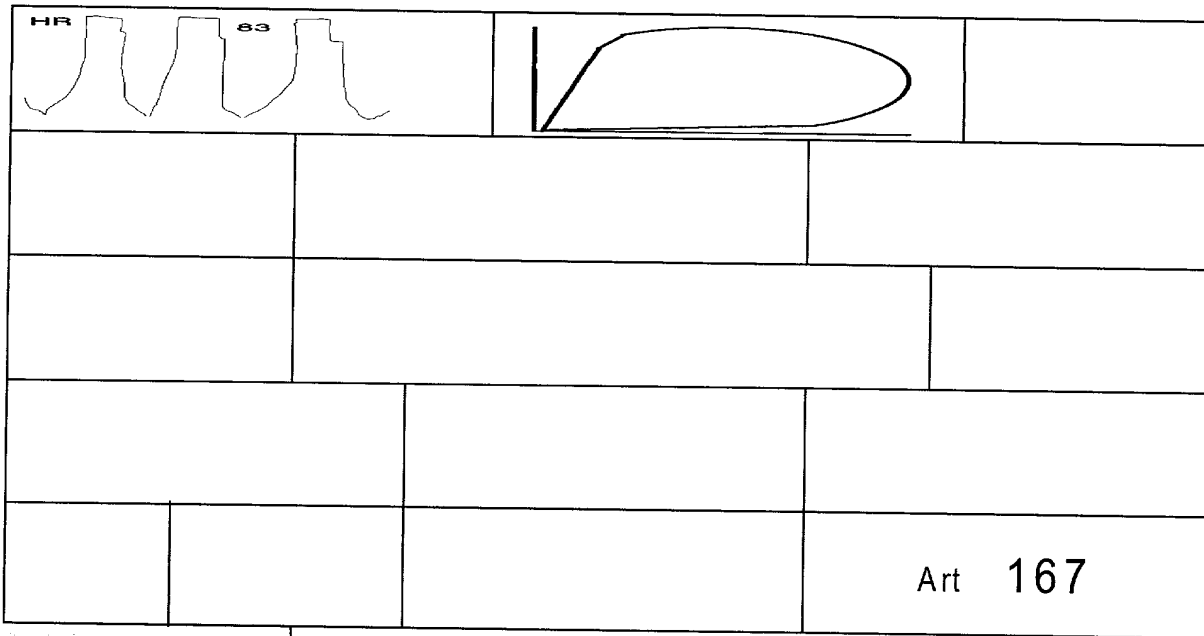

64

Fig. 13

HR 83	iO ₂ 35	iCO ₂	Temp	DO ₂	PaCO ₂
Art 167	etO ₂ 33	etCO ₂	GP 1	DO ₂ I	CvO ₂
SpO ₂ 97	RA 15	FIO ₂	GP 2	LVSW	CaO ₂
PA 33	RV	CO	PaO ₂	RVSW	
CVP 15	LA	SvO ₂	PWP		
Resp 20	LV	SaO ₂			
PIs 83	ICP				

65

Fig. 14

HR	83
ART	167/69/106
PA	33

66

Fig. 15

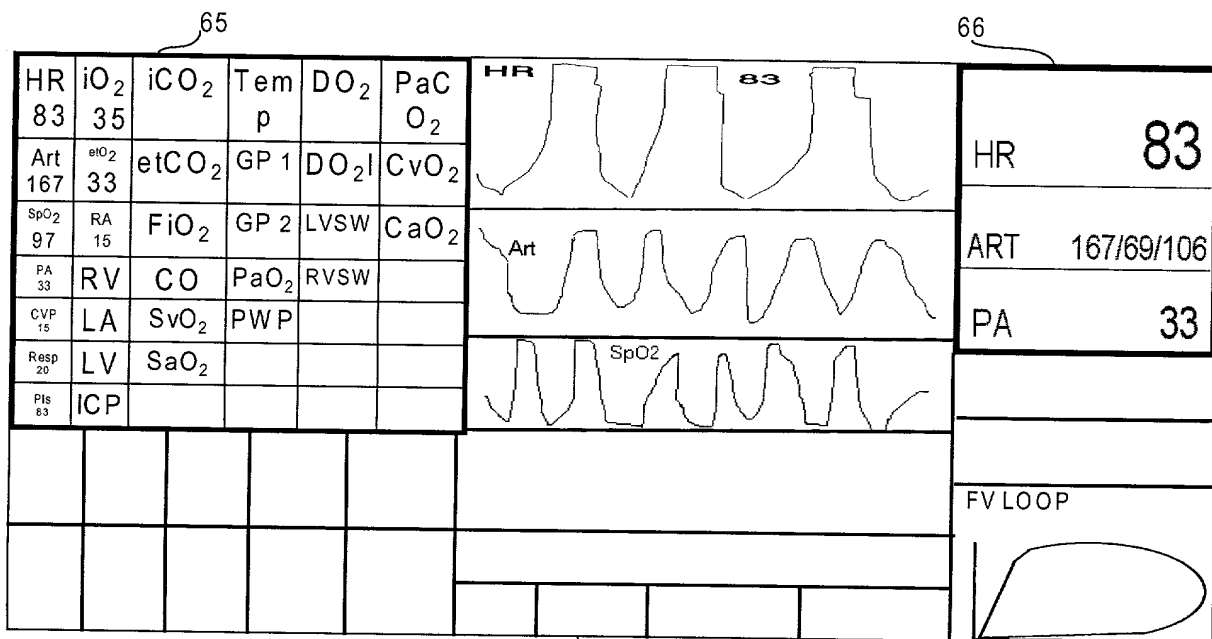


Fig. 16

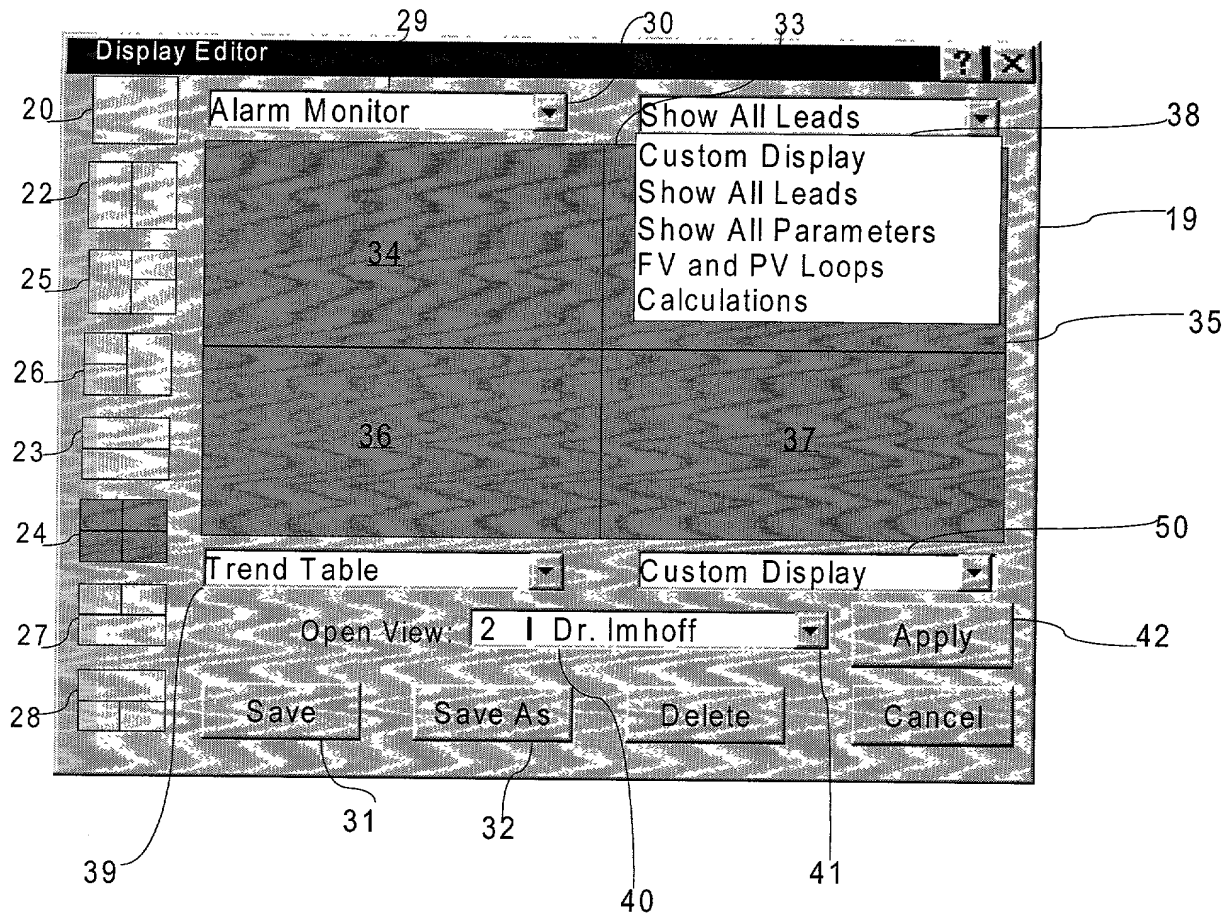


Fig. 17

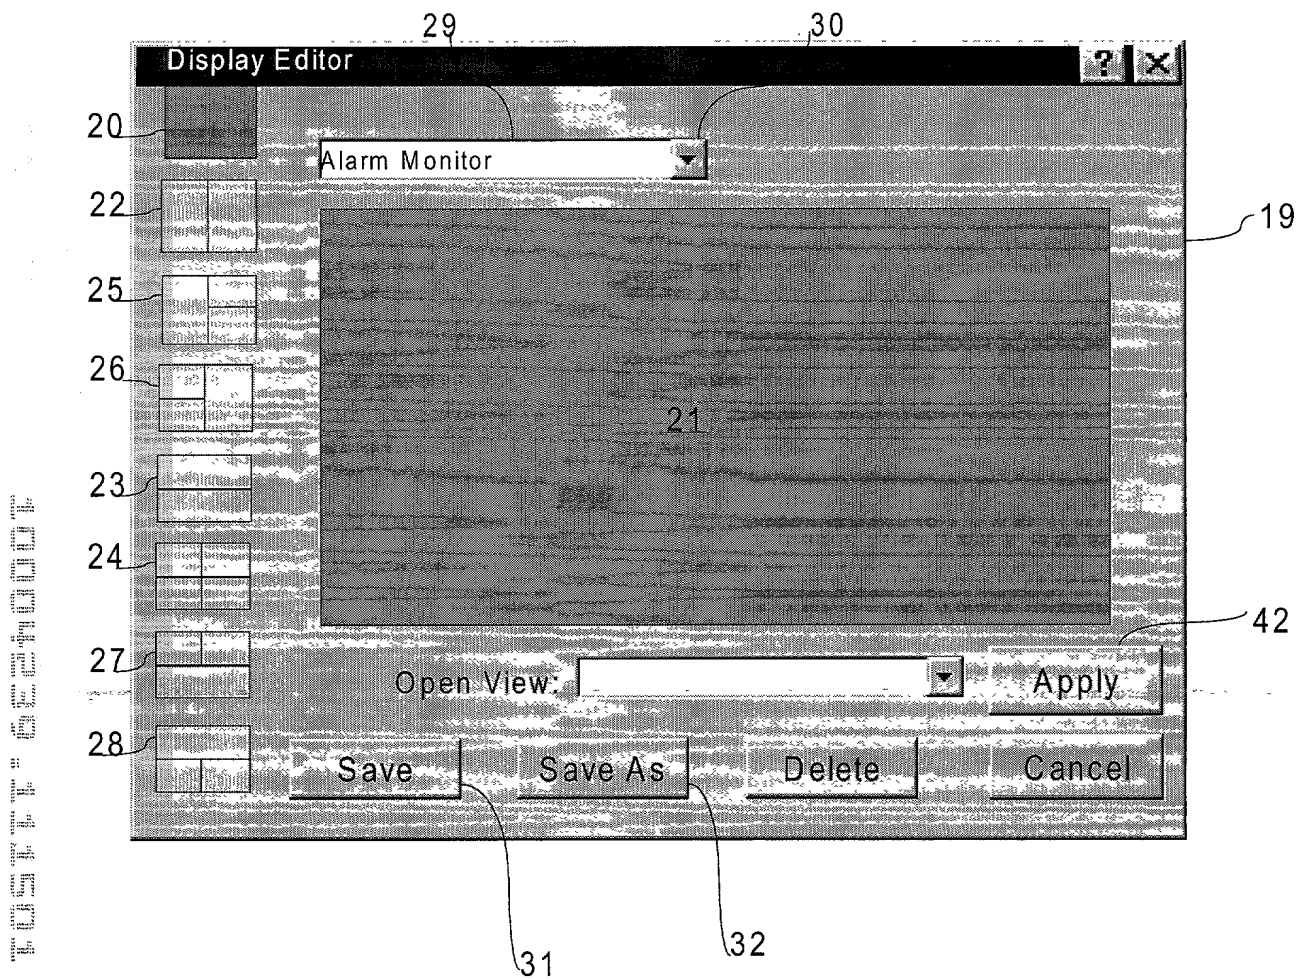


Fig. 18

Save View Layout As ? X

Choose a button and enter the view name

One Ext. View

Dr. Imhoff

Save Cancel

1

7

2

3

4

5

Fig. 19